


SURGICAL STEPS¹




STEP 01

The tube must be ligated near the tube-plate junction preferably with a 7-0 vicryl dissolvable suture to occlude the tube. One technique to occlude the tube involves the placement of a releasable ripcord in the tube lumen at the time of the initial surgery. A 4-inch, 4-0 polypropylene ripcord is provided in the tube lumen. A 7-0 vicryl dissolvable suture is placed around the tube (and consequently around the ripcord) and tightened to prevent any flow through the tube and around the ripcord.

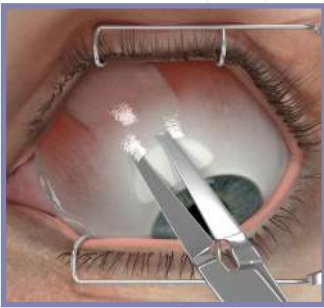



STEP 02

A conjunctival peritomy incision is made. A pocket is formed superiorly, avoiding the superior rectus and oblique muscles, by blunt dissection of Tenon's capsule from the episclera.

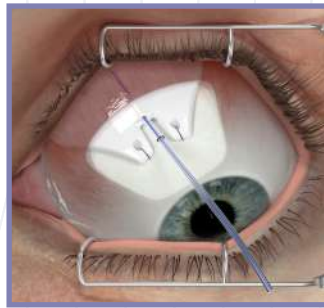


STEP 03

The implant is placed away from the limbus under the conjunctiva and Tenon's capsule between the rectus muscles (the endplate of the model 350 is wider than the model 250 endplate and has portions that fit under adjacent rectus muscles) and sutured to the episclera. The leading edge of the endplate should be ~ 8-10 mm from the limbus resulting in the suture arms being 6-8 mm from the limbus when implanted in the superior quadrants or 4-6 mm when implanted in the inferior quadrants.

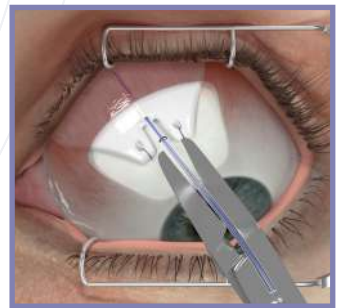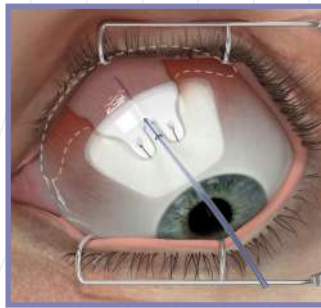


STEP 04

The drainage tube is trimmed to permit a 2-3 mm insertion of the tube into the anterior chamber (AC). The tube should be bevel cut to an anterior angle of 30° to facilitate insertion.

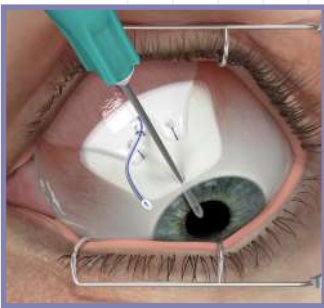

STEP 05

The AC is entered at 2-3 mm from the limbus with a sharp 23-gauge needle to create a needle track, parallel to the iris. In addition, a paracentesis should be performed to allow for quick AC reformation in case of a flattened AC.

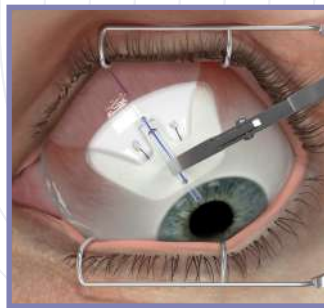

STEP 06

The drainage tube is inserted approximately 2-3 mm into the AC through the needle track, created in Step 5.

STEP 07

After surgery, the body's wound healing mechanism results in the formation of a fibrous capsule (bleb) composed of scar tissue around the implant, this scar tissue resists fluid outflow. In approximately 4-6 weeks the 7-0 vicryl suture dissolves. At that time, under a magnified view of a slit lamp biomicroscope or operating microscope the conjunctiva can be entered over the temporal side of the ripcord and the ripcord can be removed using jeweler's forceps. Following the ripcord removal, the IOP should be checked and slit lamp and fundoscopic examination should be performed.

The steps illustrated here are intended as a guideline only, and do not represent recommended treatment for any particular patient. The use of any specific surgical technique or maneuver is at the sole discretion of the surgeon. Surgeons should be familiar with the use of glaucoma drainage devices and post-operative care considerations before implanting any drainage device. Reference papers and surgical videos are available upon request.

WHY AHMED CLEARPATH® ?

ADDRESSING MARKET DEMANDS WITH A TRUSTED BRAND

OPTIMIZED PLATE DESIGN

Allows for a true single quadrant implantation and avoids rectus muscle isolation (CP250). Winged design (CP350) avoids rectus muscle attachment points

GLOBE-CONFORMING FLEXIBLE MATERIAL

Allows the globe-shaped implant to provide a more natural fit while providing a low-lying diffused bleb



FIXATION EYELETS

Easier access for suturing plate and allows for a more posterior plate placement

ALL-INCLUSIVE PACKAGING

Includes a pre-packaged ripcord and needle for scleral track

PRE-THREADED RIPCORD SUTURE

Allows options for IOP management post-surgery

Ahmed
CLEARPATH®



Ready to get
Started?

Join LEARN, our online training platform
to instantly gain access to product
education and training modules

 **NEW WORLD**
MEDICAL

References-

1. New World Medical. (2025, March). The Ahmed ClearPath® Glaucoma Drainage Device IFU. <https://www.learn.newworldmedical.com/wp-content/uploads/2025/03/50-0184-IFU-CLEARPATH-ARTWORK-MULTILINGUAL-WEB-VERSION.pdf>